

Company: Lamont Doherty

Well: ODP Leg 204, Site 1250F

Field: Hydrate Ridge

Ocean: Pacific State: Oregon

Phasor Induction

Natural Gamma Ray (Tcombo)

Ocean: Pacific
Field: Hydrate Ridge
Location: W 125* 9.0064'
Well: ODP Leg 204, Site 1250F
Company: Lamont Doherty

Table with columns: LOCATION, Permanent Datum, Log Measured From, Drilling Measured From, API Serial No., Max. Hole Devi., Longitude, Latitude. Includes coordinates W 125* 9.0064', N 44* 34.1162', and elevations.

Main data table with columns: Logging Date, Run Number, Depth Driller, Schlumberger Depth, Bottom Log Interval, Top Log Interval, Casing Driller Size @ Depth, Casing Schlumberger, Bit Size, Type Fluid In Hole, Density, Fluid Loss, Source Of Sample, RM @ Measured Temperature, RMC @ Measured Temperature, Source RMF, RM @ MRT, Maximum Recorded Temperatures, Circulation Stopped, Logger On Bottom, Unit Number, Recorded By, Witnessed By.

Summary table with columns: Logging Date, Run Number, Depth Driller, Schlumberger Depth, Bottom Log Interval, Top Log Interval, Casing Driller Size @ Depth, Casing Schlumberger, Bit Size, Type Fluid In Hole, Density, Fluid Loss, Source Of Sample, RM @ Measured Temperature, RMC @ Measured Temperature, Source RMF, RM @ MRT, Maximum Recorded Temperatures, Circulation Stopped, Logger On Bottom, Unit Number, Recorded By, Witnessed By. Includes 'Run 1', 'Run 2', and 'Run' labels.

DISCLAIMER

THE USE OF AND RELIANCE UPON THIS RECORDED-DATA BY THE HEREIN NAMED COMPANY (AND ANY OF ITS AFFILIATES, PARTNERS, REPRESENTATIVES, AGENTS, CONSULTANTS AND EMPLOYEES) IS SUBJECT TO THE TERMS AND CONDITIONS AGREED UPON BETWEEN SCHLUMBERGER AND THE COMPANY, INCLUDING: (a) RESTRICTIONS ON USE OF THE RECORDED-DATA; (b) DISCLAIMERS AND WAIVERS OF WARRANTIES AND REPRESENTATIONS REGARDING COMPANY'S USE OF AND RELIANCE UPON THE RECORDED-DATA; AND (c) CUSTOMER'S FULL AND SOLE RESPONSIBILITY FOR ANY INFERENCE DRAWN OR DECISION MADE IN CONNECTION WITH THE USE OF THIS RECORDED-DATA.




OTHER SERVICES1 OS1: FMS/DSST OS2: VSI OS3: IPLT/DITE OS4: OS5:	OTHER SERVICES2 OS1: OS2: OS3: OS4: OS5:
--	---


REMARKS: RUN NUMBER 1 All depths measured in meters below rig floor.	REMARKS: RUN NUMBER 2
Sea Floor SLB 807 mbrf. Drill pipe SLB 863 mbrf.	
Drill pipe affects after calibration for DITE.	

RUN 1			RUN 2		
SERVICE ORDER #:			SERVICE ORDER #:		
PROGRAM VERSION:	10C0-306		PROGRAM VERSION:		
FLUID LEVEL:			FLUID LEVEL:		
LOGGED INTERVAL	START	STOP	LOGGED INTERVAL	START	STOP

EQUIPMENT DESCRIPTION

RUN 1		RUN 2	
SURFACE EQUIPMENT			
SFT-281 24 SFT-178 4722 GSR-U 135 WITM (DTS)-A			

DOWNHOLE EQUIPMENT			
LEH-QT			34.84
LEH-QT 1497			
AH-QSST			33.95
AH-QSST 12			
DTC-H		CTEM TelStatus ToolStatu	32.30
ECH-KC 9841			31.66
			32.58

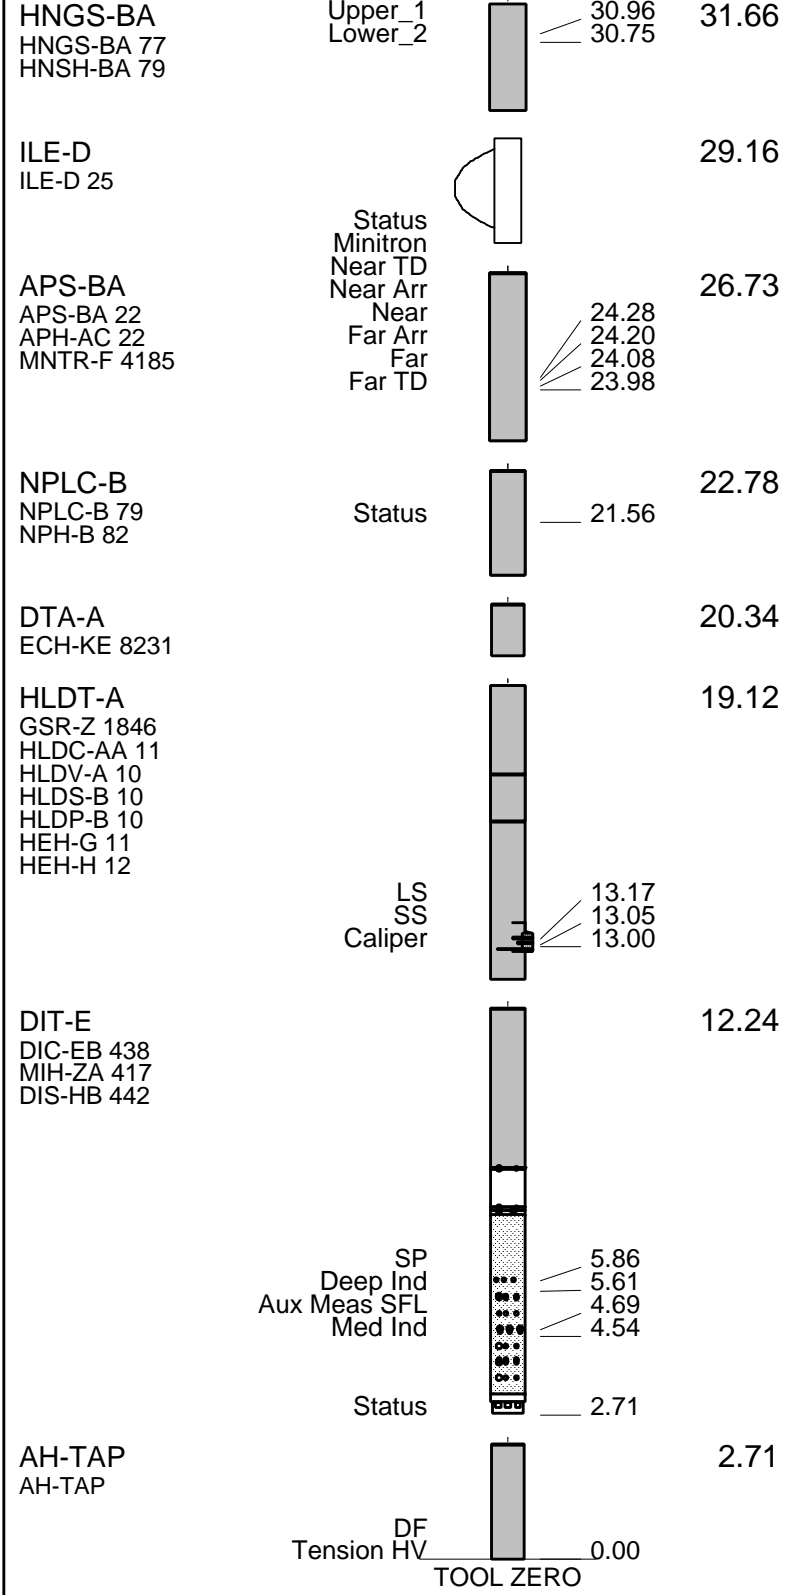

TOOL ZERO

MAXIMUM STRING DIAMETER 3.88 IN
 MEASUREMENTS RELATIVE TO TOOL ZERO
 ALL LENGTHS IN METERS

Output DLIS Files


DEFAULT	PI_LDL_APS_NGS_005LUP	FN:7	PRODUCER	25-Aug-2002 21:57	985.3 M	784.1 M
REDUCE	PI_LDL_APS_NGS_005LUP	FN:8	PRODUCER	25-Aug-2002 21:57	985.3 M	784.1 M


OP System Version: 10C0-306 MCM


DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

PIP SUMMARY

Time Mark Every 60 S

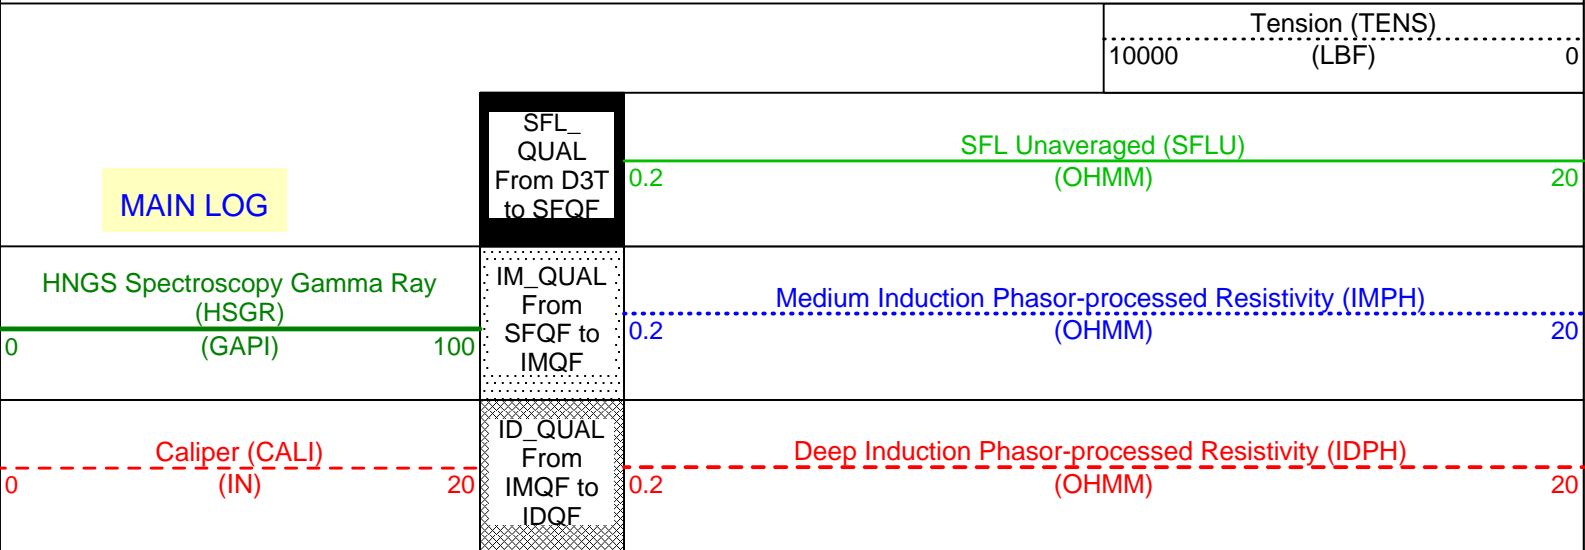

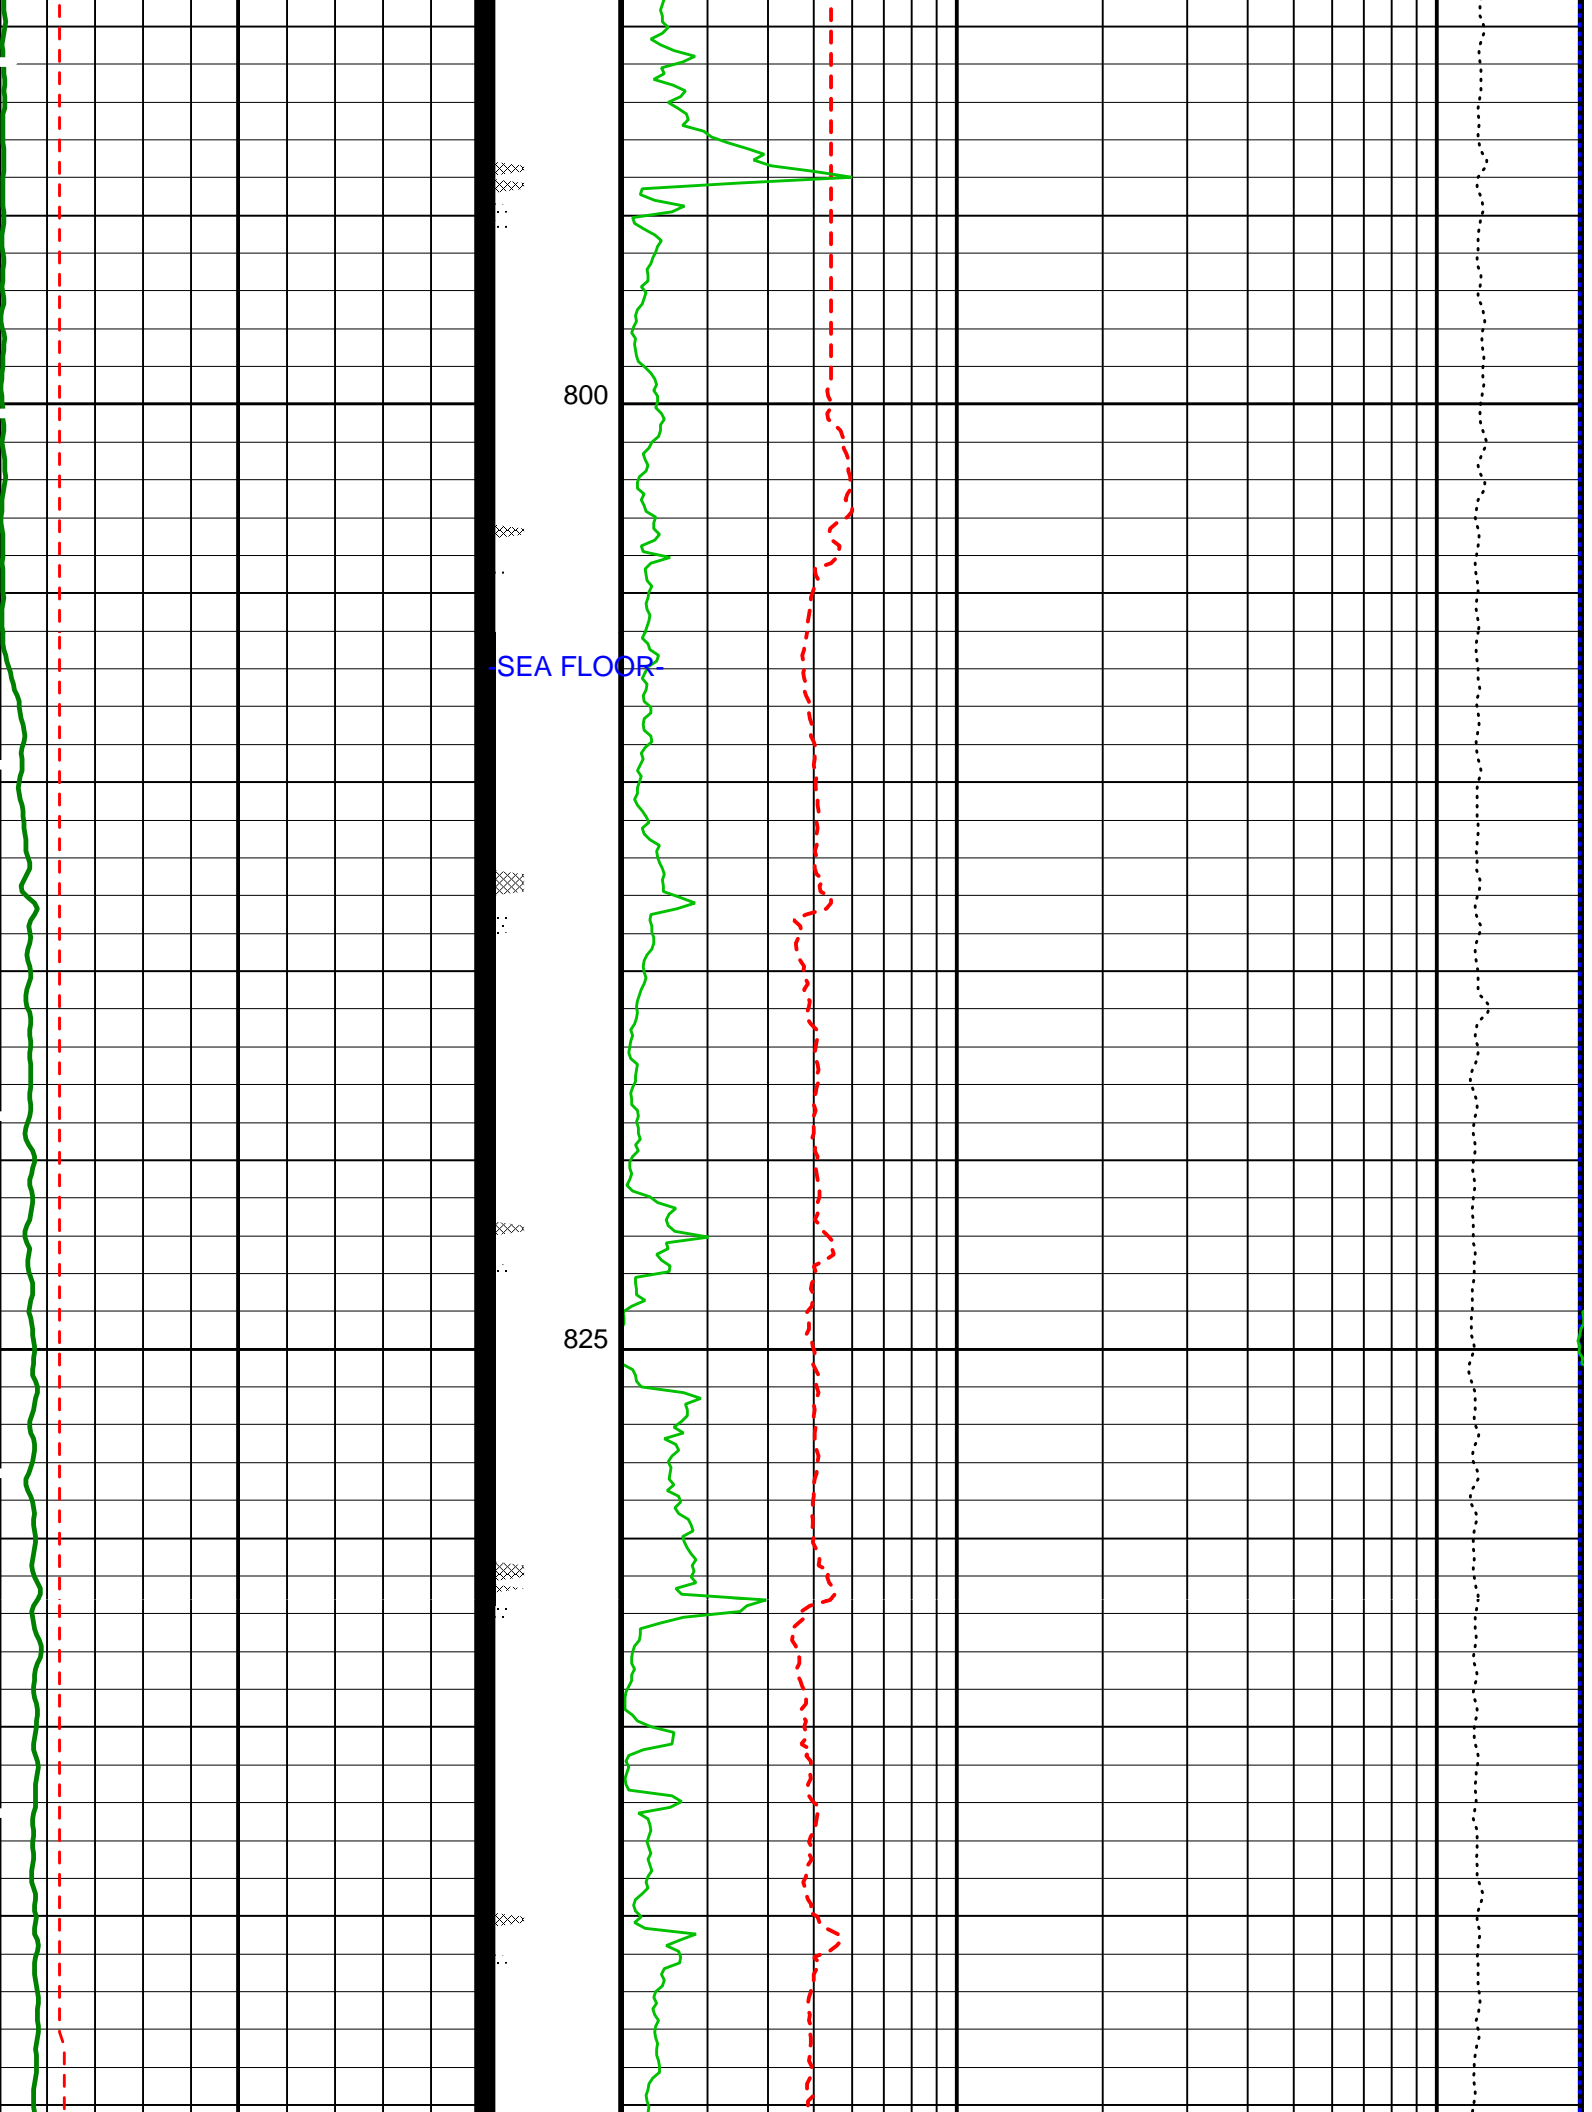

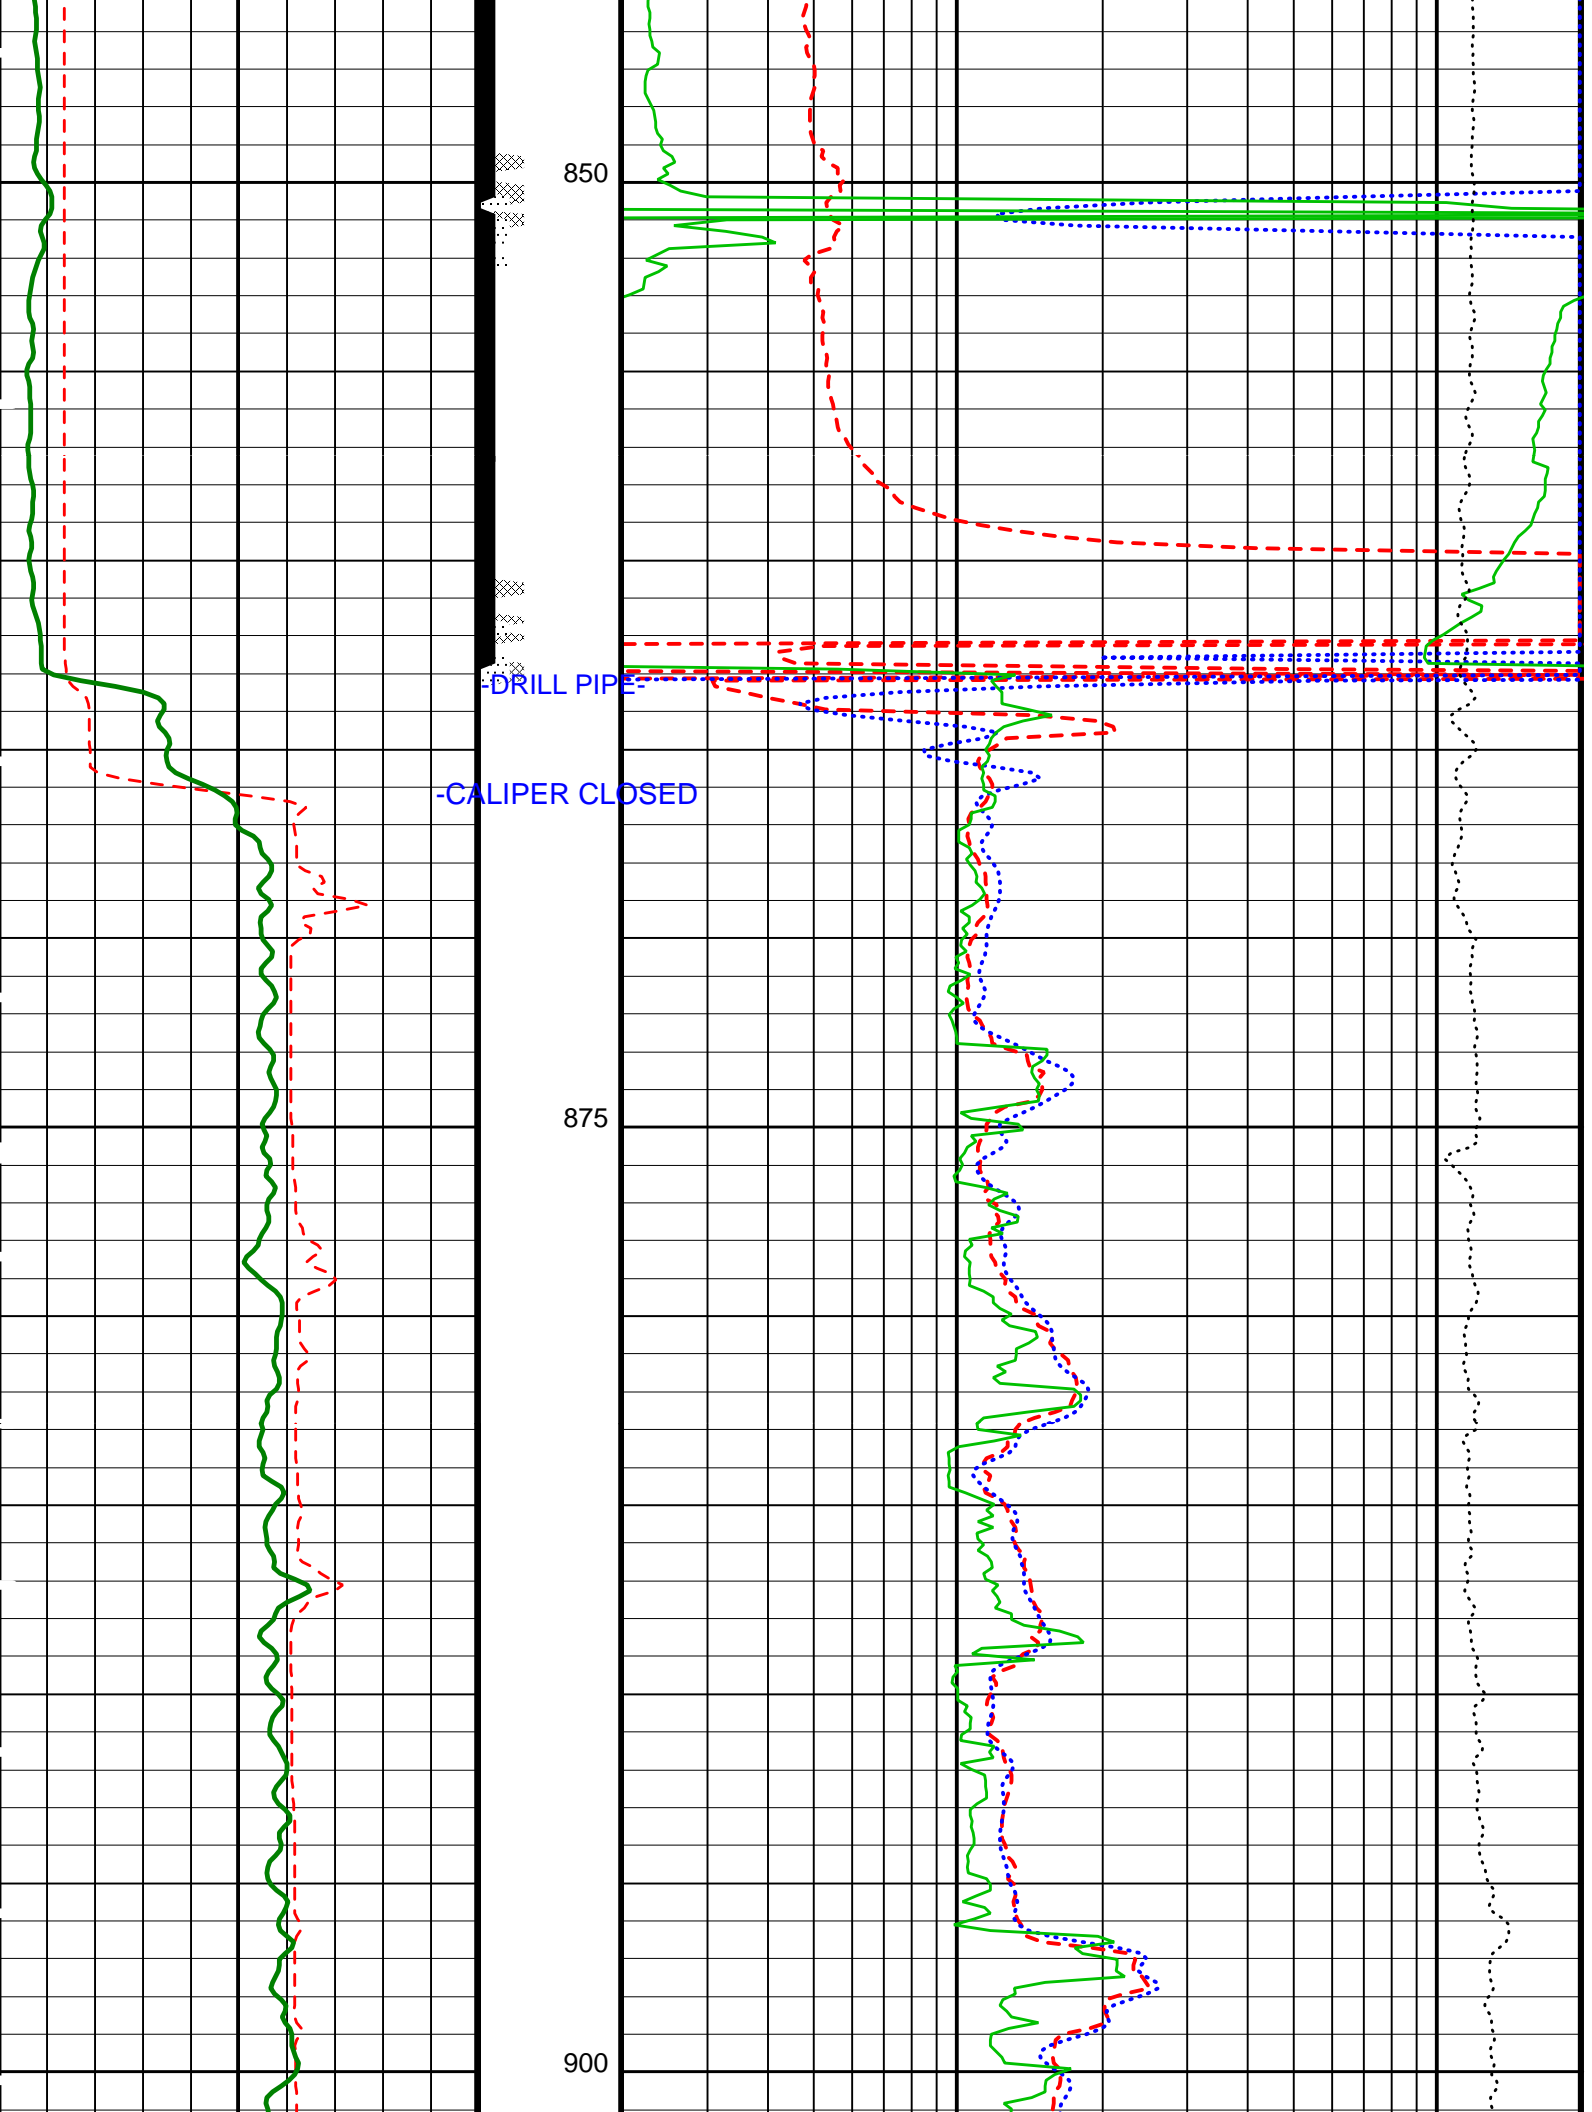


850


DRILL PIPE

-CALIPER CLOSED

875

900

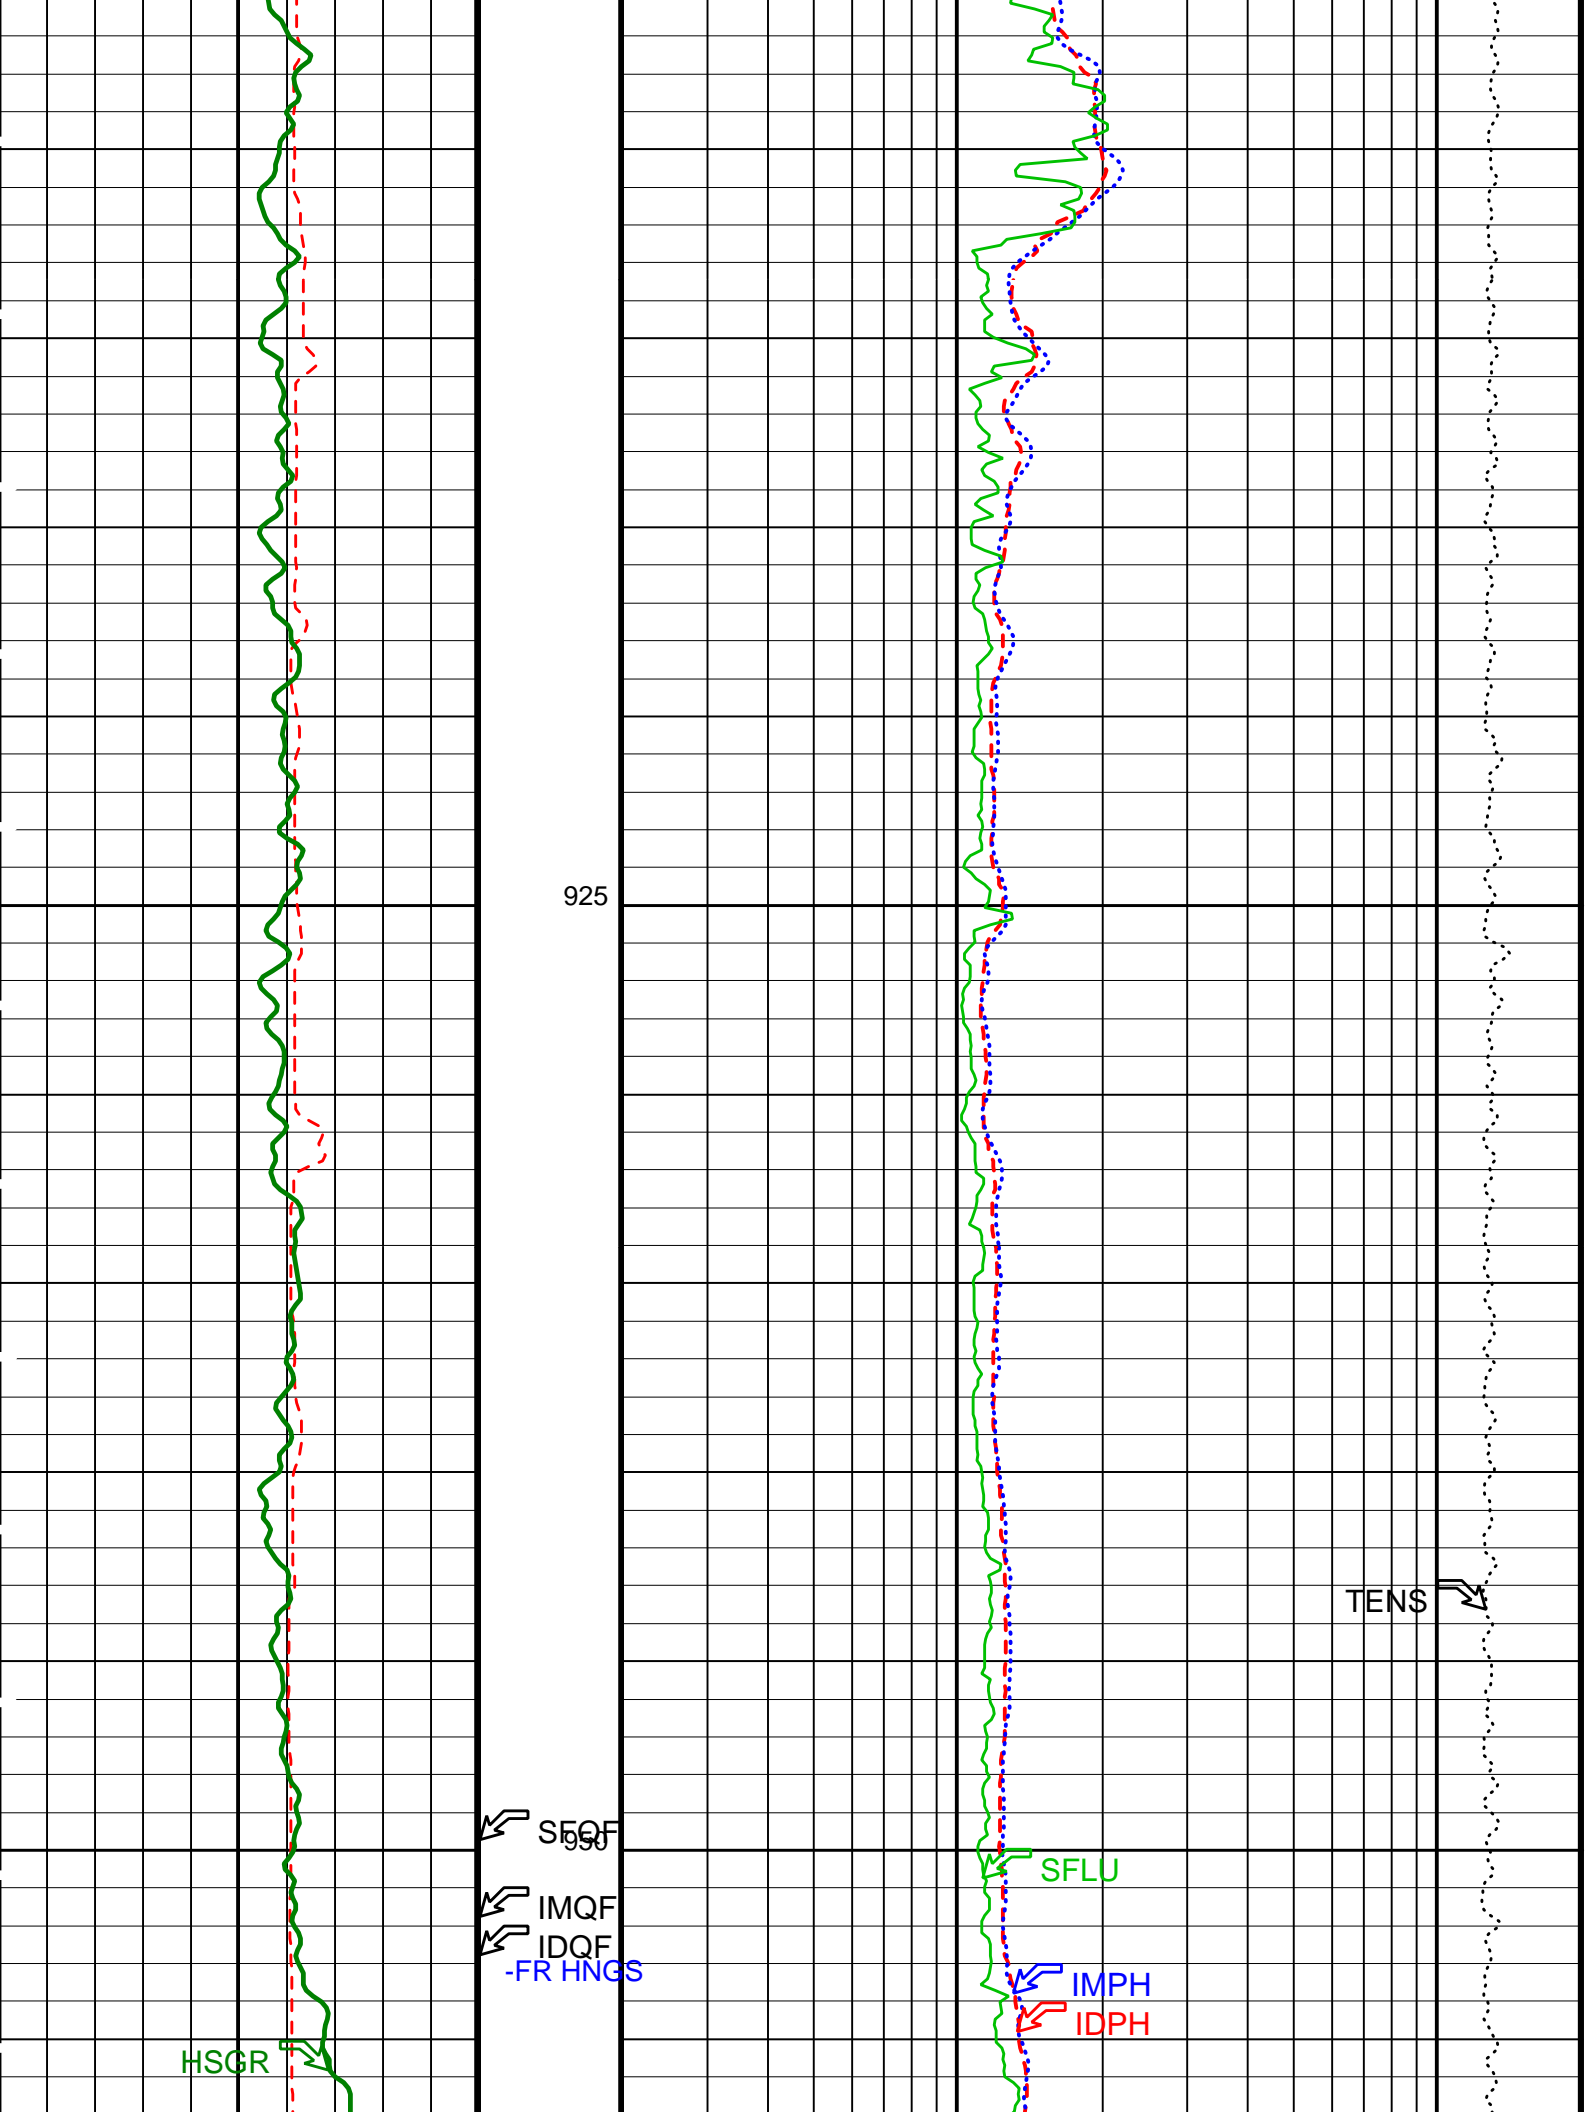

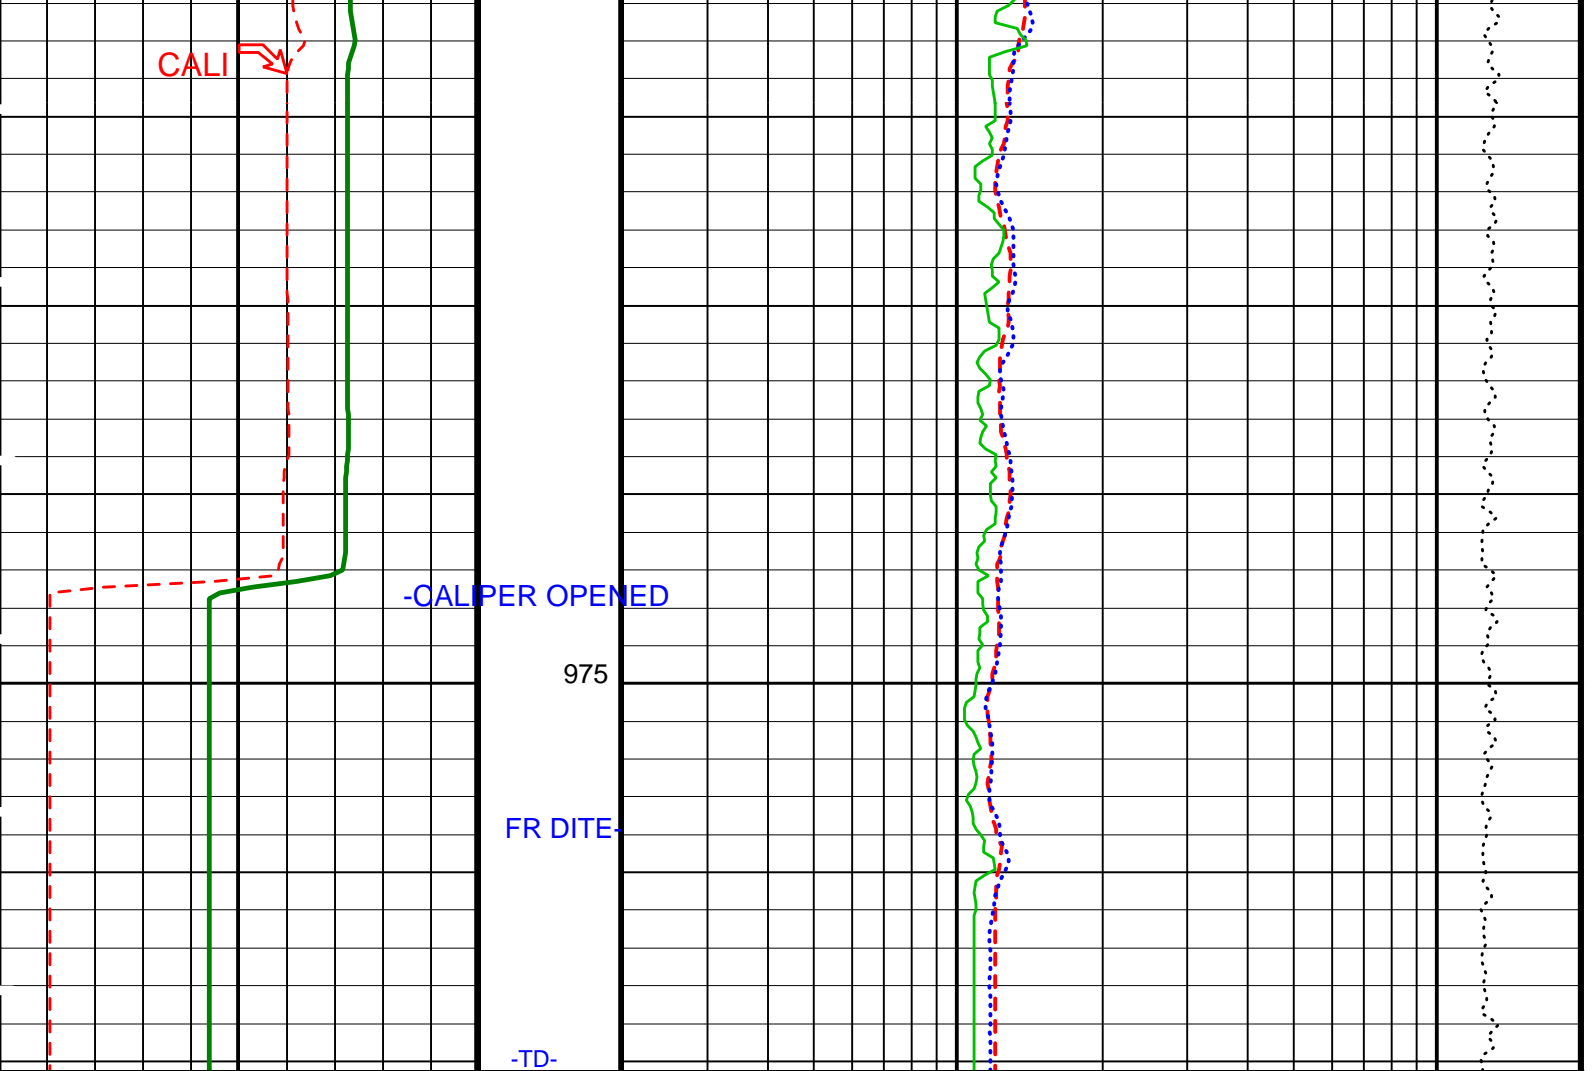

Caliper (CALI) (IN)	ID_QUAL From IMQF to IDQF	Deep Induction Phasor-processed Resistivity (IDPH) (OHMM)
HNGS Spectroscopy Gamma Ray (HSGR) (GAPI)	IM_QUAL From SFQF to IMQF	Medium Induction Phasor-processed Resistivity (IMPH) (OHMM)
MAIN LOG	SFL_QUAL From D3T to SFQF	SFL Unaveraged (SFLU) (OHMM)
		Tension (TENS) (LBF)

PIP SUMMARY

Time Mark Every 60 S

Parameters

DLIS Name	Description	Value
DIT-E: Dual Induction - E		
BHS	Borehole Status	OPEN
BHT	Bottom Hole Temperature (used in calculations)	100 DEGC
DGF2	Deep 20 kHz Gain Factor	1.00789
DPH2	Deep 20 kHz Phase Shift	-0.152394 DEG
DRE2	Deep Real 20 kHz Sonde Error Correction	16.357 MM/M
DSR2	Deep Sigma Reference (20 kHz)	1843 MM/M
DXE2	Deep Quad 20 kHz Sonde Error Correction	64.6326 MM/M
GCSE	Generalized Caliper Selection	CALI
GDEV	Average Angular Deviation of Borehole from Normal	0 DEG
GGRD	Geothermal Gradient	0.018227 DC/M

GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
IFRS	DIT-E Induction Frequency Selector	20	
IPHA	DIT-E Phasor Processing Mode	ALL	
IPRO	DIT-E Induction Processing Selector	PHASOR	
ITEN	DIT-E Temperature Enable	ENABLE	
MGF2	Medium 20 kHz Gain Factor	1.02964	
MPH2	Medium 20 kHz Phase Shift	-0.933067	DEG
MRE2	Medium Real 20 kHz Sonde Error Correction	-1.78642	MM/M
MSR2	Medium Sigma Reference (20 kHz)	3250	MM/M
MXE2	Medium Quad 20 kHz Sonde Error Correction	-34.2041	MM/M
SFCR	SFL Channel Ratio	1000	
SHT	Surface Hole Temperature	20	DEGC
APS-BA: Accelerator-Porosity Tool			
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
SHT	Surface Hole Temperature	20	DEGC
HNGS-BA: Hostile Natural Gamma Ray Sonde			
BAR1	HNGS Detector 1 Barite Constant	1	
BAR2	HNGS Detector 2 Barite Constant	1	
BHK	HNGS Borehole Potassium Correction Concentration	0	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
CSD1	Inner Casing Outer Diameter	0	IN
CSD2	Outer Casing Outer Diameter	0	IN
CSW1	Inner Casing Weight	0	LB/F
CSW2	Outer Casing Weight	0	LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE	
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW	
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW	
HABK	HNGS Borehole Potassium Running Average	-0.00756454	
HALF	HNGS Alpha Filter Length	60	IN
HCRB	HNGS Apply Borehole Potassium Correction	NONE	
HMWM	Mud Weighting Material	NATU	
HNPE	HNGS Processing Enable	YES	
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	1.3	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	1.3	CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES	
SHT	Surface Hole Temperature	20	DEGC
TPOS	Tool Position	ECCE	
VBA1	HNGS Detector 1 Variable Barite Factor Running Average	0.961934	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	0.981195	
System and Miscellaneous			
BS	Bit Size	11.438	IN
DFD	Drilling Fluid Density	1.10	G/C3
TD	Total Depth	-50000	M

Format: DITE_LogPhasor Vertical Scale: 1:200 Graphics File Created: 25-Aug-2002 21:57

OP System Version: 10C0-306

MCM

DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_005LUP	FN:7	PRODUCER	25-Aug-2002 21:57
REDUCE	PI_LDL_APS_NGS_005LUP	FN:8	PRODUCER	25-Aug-2002 21:57

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_006LUP	FN:9	PRODUCER	25-Aug-2002 22:37	985.3 M	853.9 M
REDUCE	PI_LDL_APS_NGS_006LUP	FN:10	PRODUCER	25-Aug-2002 22:37	985.3 M	853.9 M

OP System Version: 10C0-306

MCM

DIT-E	10C0-306	HLDT-A	10C0-306
-------	----------	--------	----------



PIP SUMMARY

Time Mark Every 60 S





REPEAT SECTION



SFL_QUAL
From D3T
to SFQF

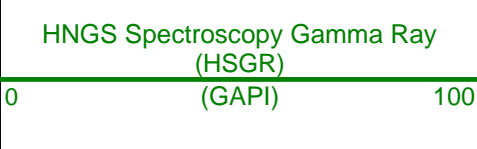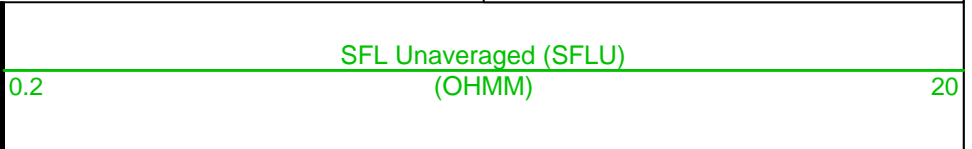



IM_QUAL
From SFQF
to IMQF

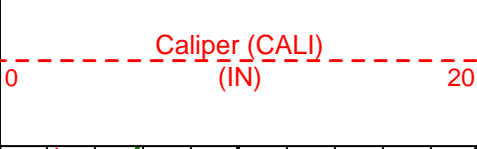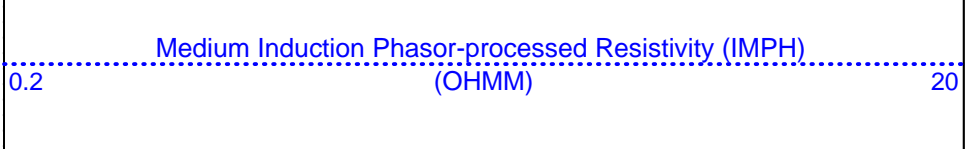

ID_QUAL
From IMQF
to IDQF

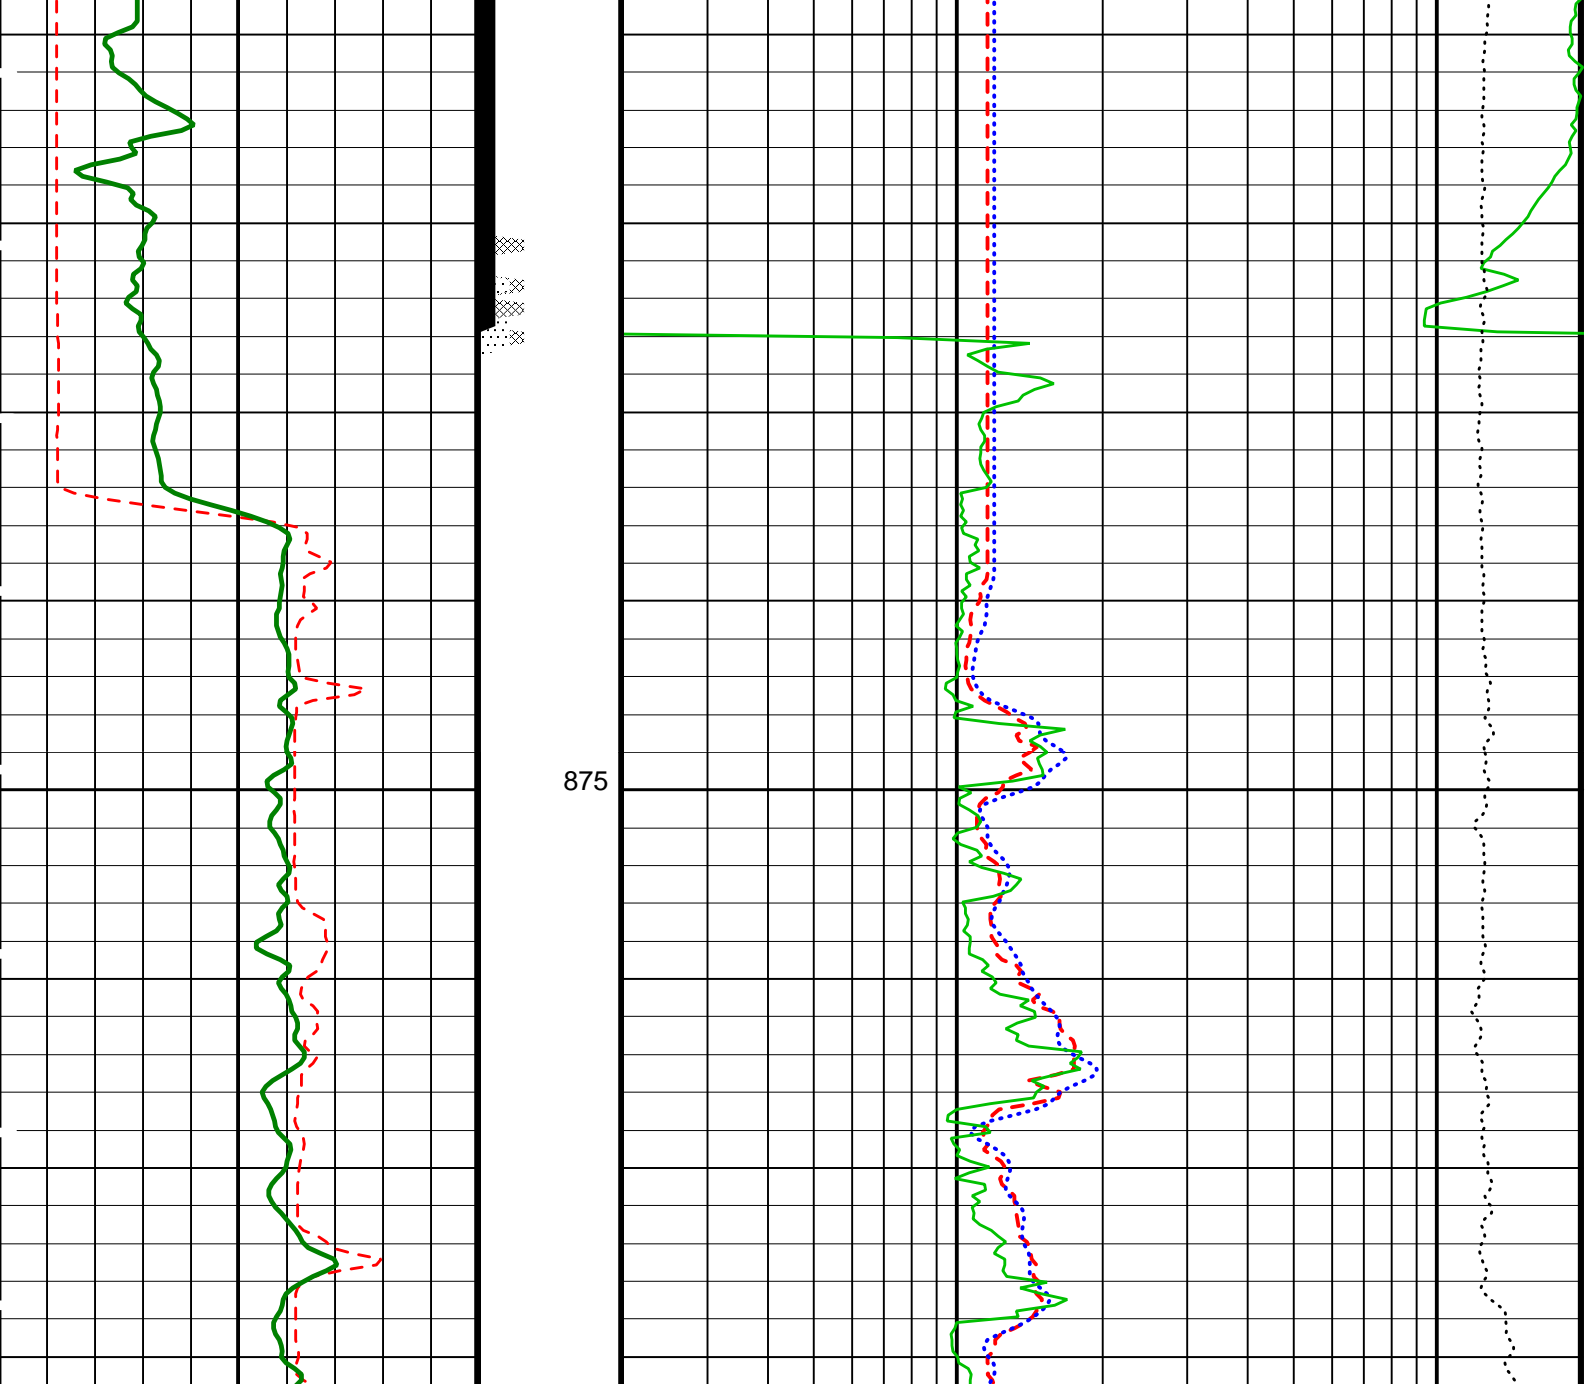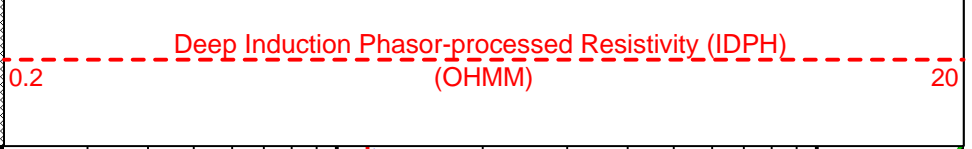

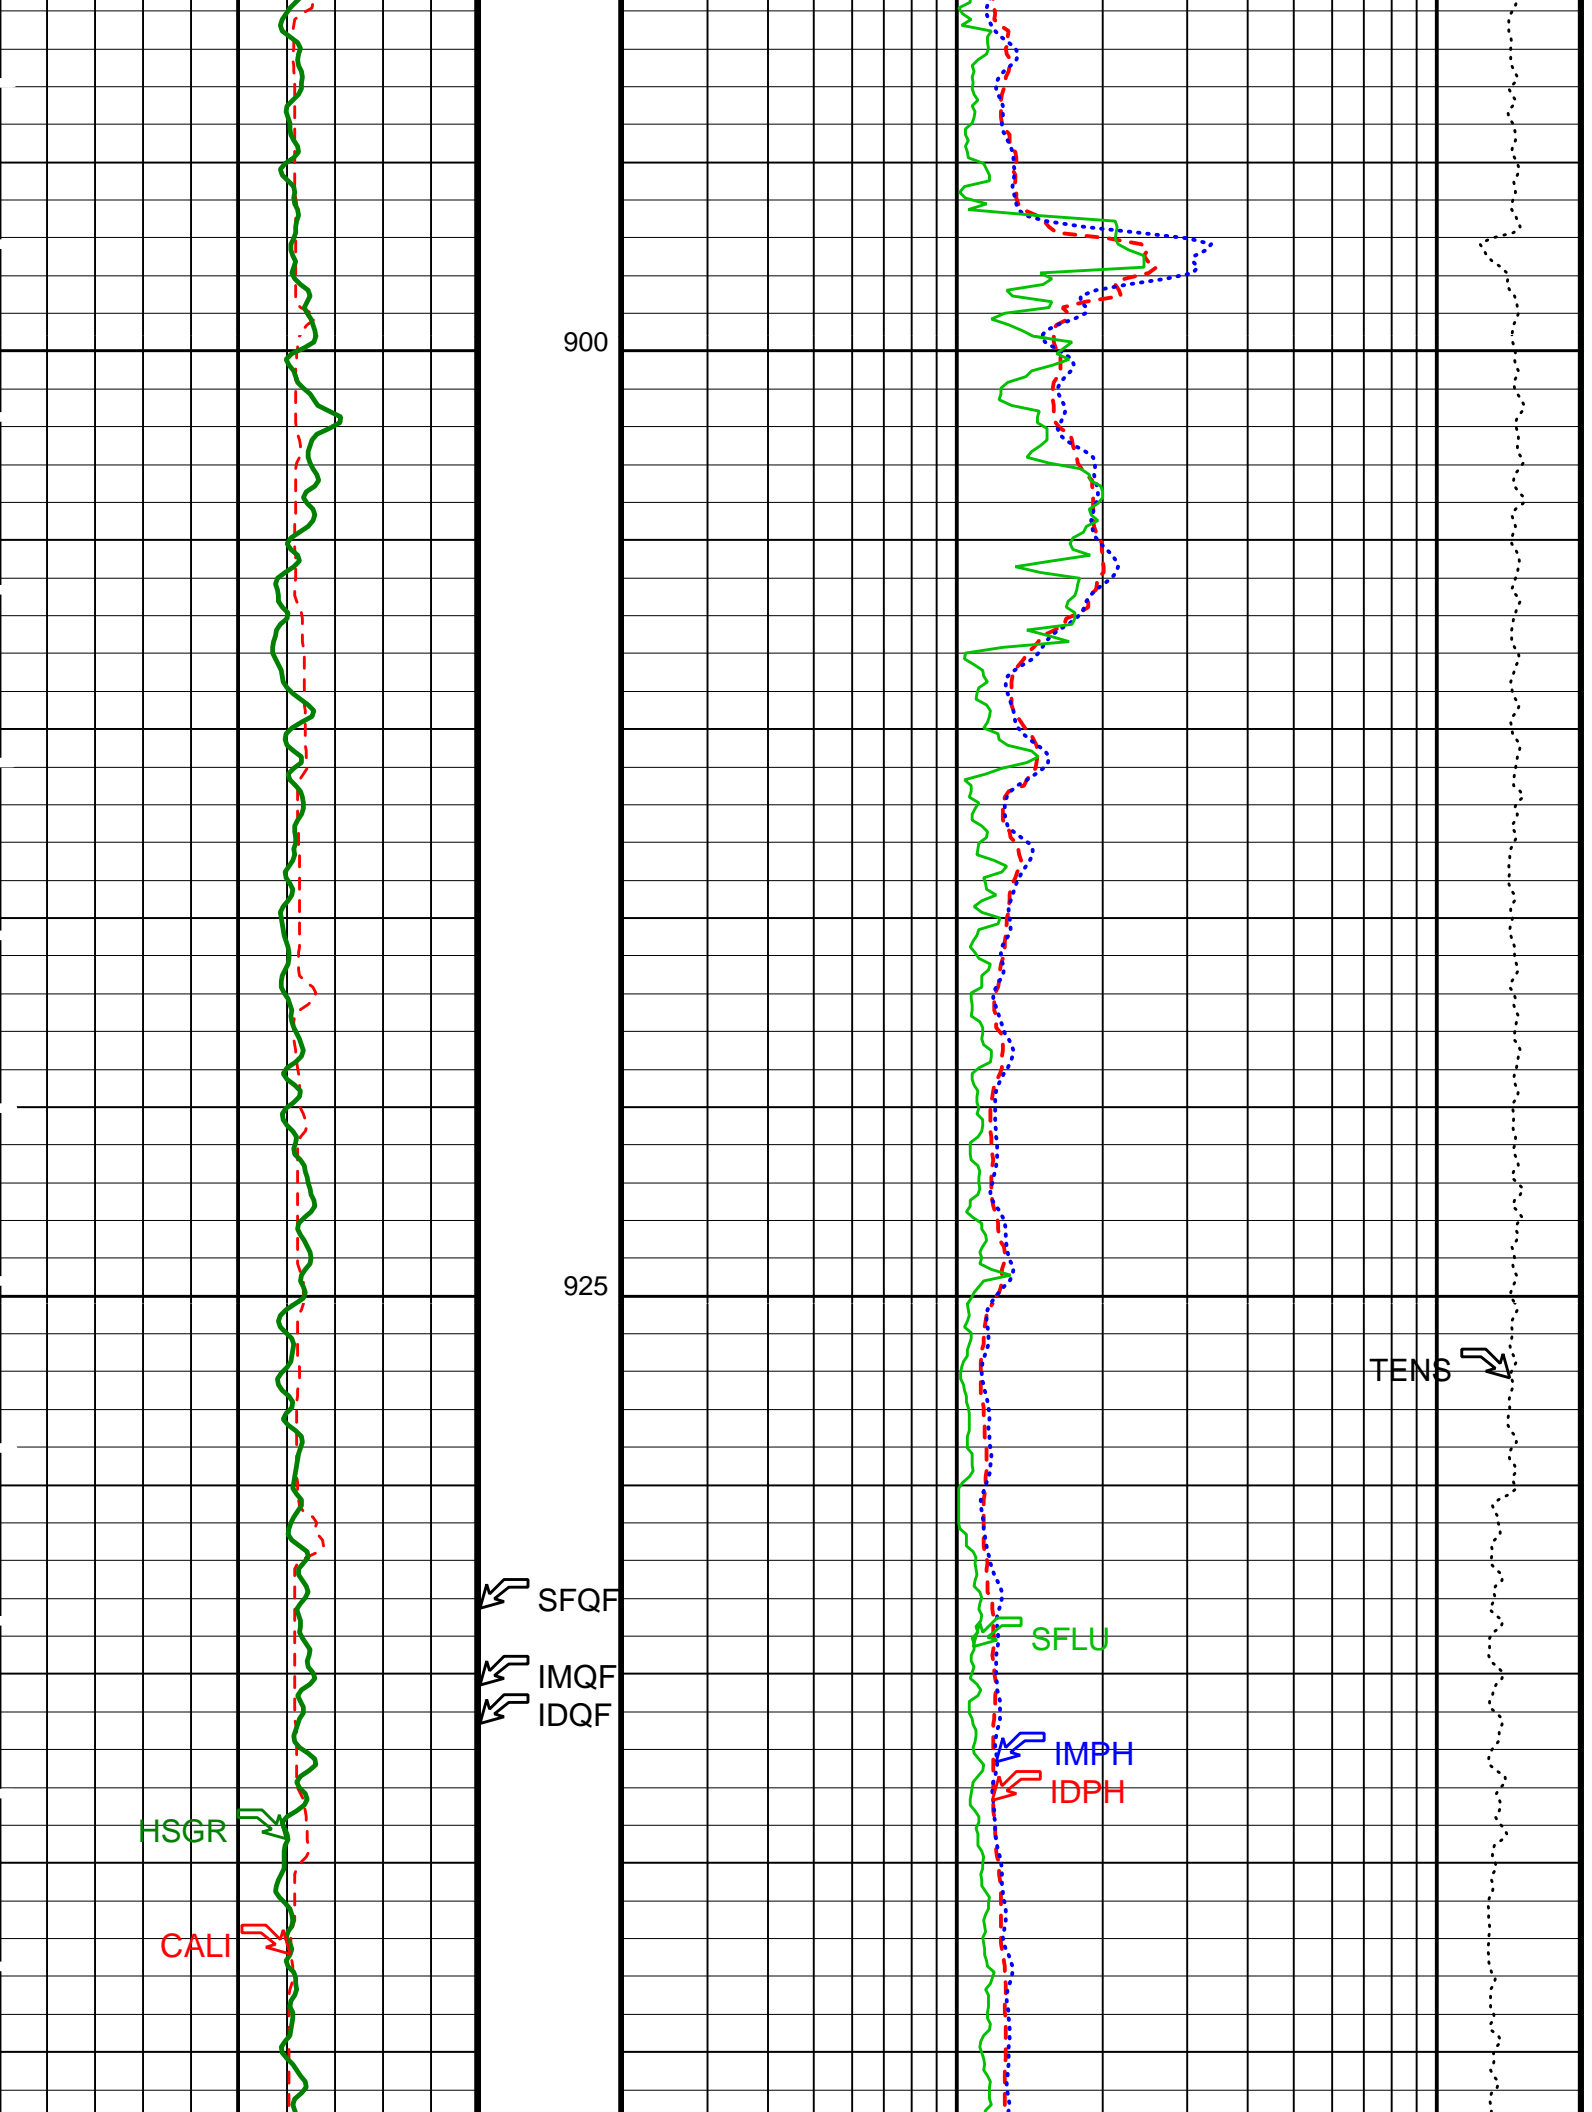

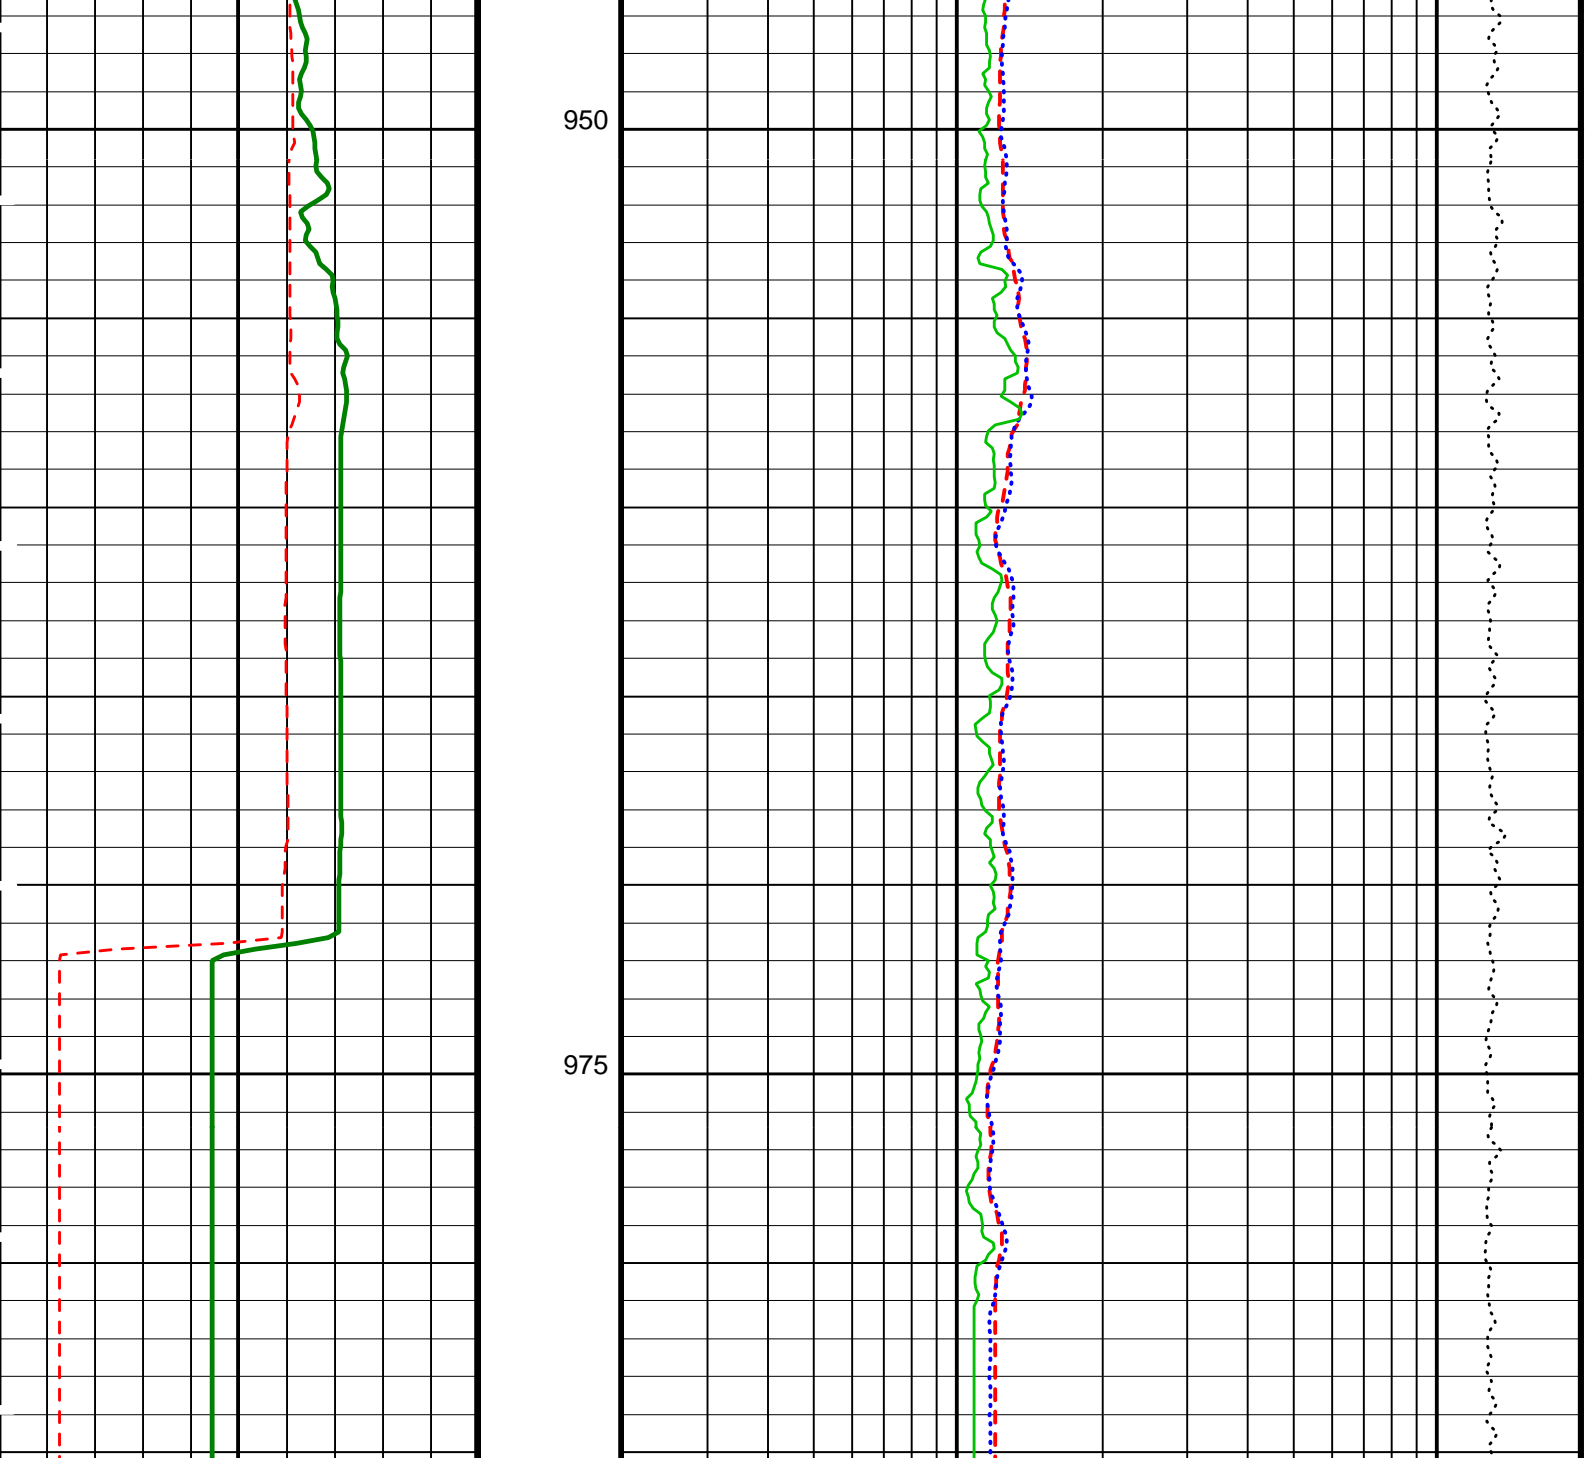

<p>Caliper (CALI) (IN)</p> <p>0 20</p>	<p>ID_QUAL From IMQF to IDQF</p>	<p>Deep Induction Phasor-processed Resistivity (IDPH) (OHMM)</p> <p>0.2 20</p>
<p>HNGS Spectroscopy Gamma Ray (HSGR) (GAPI)</p> <p>0 100</p>	<p>IM_QUAL From SFQF to IMQF</p>	<p>Medium Induction Phasor-processed Resistivity (IMPH) (OHMM)</p> <p>0.2 20</p>
<p>REPEAT SECTION</p>	<p>SFL_QUAL From D3T to SFQF</p>	<p>SFL Unaveraged (SFLU) (OHMM)</p> <p>0.2 20</p>
		<p>Tension (TENS) (LBF)</p> <p>10000 0</p>

PIP SUMMARY

Time Mark Every 60 S

Parameters

DLIS Name	Description	Value	
DIT-E: Dual Induction - E			
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
DGF2	Deep 20 kHz Gain Factor	1.00789	
DPH2	Deep 20 kHz Phase Shift	-0.152394	DEG
DRE2	Deep Real 20 kHz Sonde Error Correction	16.357	MM/M
DSR2	Deep Sigma Reference (20 kHz)	1843	MM/M
DXE2	Deep Quad 20 kHz Sonde Error Correction	64.6326	MM/M
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
IFRS	DIT-E Induction Frequency Selector	20	
IPHA	DIT-E Phasor Processing Mode	ALL	
IPRO	DIT-E Induction Processing Selector	PHASOR	
ITEN	DIT-E Temperature Enable	ENABLE	
MGF2	Medium 20 kHz Gain Factor	1.02964	
MPH2	Medium 20 kHz Phase Shift	-0.933067	DEG
MRE2	Medium Real 20 kHz Sonde Error Correction	-1.78642	MM/M
MSR2	Medium Sigma Reference (20 kHz)	3250	MM/M
MXE2	Medium Quad 20 kHz Sonde Error Correction	-34.2041	MM/M
SFCR	SFL Channel Ratio	1000	
SHT	Surface Hole Temperature	20	DEGC
APS-BA: Accelerator-Porosity Tool			
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
SHT	Surface Hole Temperature	20	DEGC
HNGS-BA: Hostile Natural Gamma Ray Sonde			
BAR1	HNGS Detector 1 Barite Constant	1	
BAR2	HNGS Detector 2 Barite Constant	1	
BHK	HNGS Borehole Potassium Correction Concentration	0	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
CSD1	Inner Casing Outer Diameter	0	IN
CSD2	Outer Casing Outer Diameter	0	IN
CSW1	Inner Casing Weight	0	LB/F
CSW2	Outer Casing Weight	0	LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE	
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW	
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW	
HABK	HNGS Borehole Potassium Running Average	-0.0157628	
HALF	HNGS Alpha Filter Length	60	IN
HCRB	HNGS Apply Borehole Potassium Correction	NONE	
HMWM	Mud Weighting Material	NATU	
HNPE	HNGS Processing Enable	YES	
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	1.3	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	1.3	CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES	
SHT	Surface Hole Temperature	20	DEGC
TPOS	Tool Position	ECCE	
VBA1	HNGS Detector 1 Variable Barite Factor Running Average	0.952792	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	0.948833	
System and Miscellaneous			
BS	Bit Size	11.438	IN
DFD	Drilling Fluid Density	1.10	G/C3
TD	Total Depth	-50000	M

Format: DITE_LogPhasor Vertical Scale: 1:200 Graphics File Created: 25-Aug-2002 22:37

OP System Version: 10C0-306 MCM

DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

Output DLIS Files

DEFAULT PI_LDL_APS_NGS_006LUP FN:9 PRODUCER 25-Aug-2002 22:37

Calibration and Check Summary

Measurement	Nominal	Master	Before	After	Change	Limit	Units
Hostile Environment Litho Density - A Wellsite Calibration - Background Measurement							
Master: 12-Jun-2002 0:31 Before: 24-Jul-2002 17:39 After: 20-Aug-2002 23:11							
LSW1 Background	100.0	88.67	86.74	87.05	0.3165	0.03000	CPS
LSW2 Background	105.0	93.18	91.70	90.17	-1.532	0.03000	CPS
LSW3 Background	210.0	177.4	176.2	173.3	-2.852	0.03000	CPS
LSW4 Background	290.0	236.8	236.6	234.2	-2.350	0.03000	CPS
LSW5 Background	610.0	518.0	517.3	517.7	0.3206	0.03000	CPS
SSW1 Background	100.0	83.02	84.95	84.57	-0.3811	0.03000	CPS
SSW2 Background	200.0	165.1	166.3	164.5	-1.828	0.03000	CPS
SSW3 Background	530.0	440.7	439.6	438.4	-1.202	0.03000	CPS
SSW4 Background	280.0	232.4	232.4	229.2	-3.199	0.03000	CPS
SSW5 Background	205.0	174.0	173.3	171.9	-1.433	0.03000	CPS
Hostile Environment Litho Density - A Wellsite Calibration - Tool Quality Control Information High Voltage							
Master: 12-Jun-2002 0:31 Before: 24-Jul-2002 17:39 After: 20-Aug-2002 23:11							
LS Bkg. High Voltage	1133	1133	1130	1130	0.5503	N/A	V
SS Bkg. High Voltage	1177	1177	1171	1171	-0.2373	N/A	V
Hostile Environment Litho Density - A Wellsite Calibration - Detectors Resolution From BKG Measurements							
Master: 12-Jun-2002 0:31 Before: 24-Jul-2002 17:39 After: 20-Aug-2002 23:11							
LS Background Resolution	1.000	1.032	1.032	1.031	-0.001574	N/A	
SS Background Resolution	1.000	0.9430	0.9416	0.9408	-0.0007873	N/A	
Hostile Environment Litho Density - A Wellsite Calibration - Caliper Calibration							
Before: 24-Jul-2002 17:38							
Caliper Small Ring	12.00	N/A	17.14	N/A	N/A	N/A	IN
Caliper Large Ring	15.25	N/A	21.07	N/A	N/A	N/A	IN
Accelerator-Porosity Tool Wellsite Calibration - Detector Background							
Master: 24-Jul-2002 9:08 Before: 25-Aug-2002 22:21 After: 20-Aug-2002 22:30							
Near Det Bkg Cntrate	30.00	32.30	32.55	33.34	0.7865	N/A	CPS
Far Det Bkg Cntrate	30.00	33.62	35.15	34.76	-0.3876	N/A	CPS
Array-1 Det Bkg Cntrate	30.00	28.88	28.78	29.28	0.5036	N/A	CPS
Array-2 Det Bkg Cntrate	30.00	29.64	29.62	30.01	0.3904	N/A	CPS
Array Therm Det Bkg Cntrate	30.00	32.75	32.75	32.59	-0.1626	N/A	CPS
Accelerator-Porosity Tool Wellsite Calibration - Calibration Ratios							
Master: 24-Jul-2002 9:08							
Near/Far Calibration Ratio	0.9250	0.9076	N/A	N/A	N/A	N/A	
Near/Array Calibration Ratio	1.030	1.066	N/A	N/A	N/A	N/A	
Near/Array Cal Ratio Up/Down	1.000	1.006	N/A	N/A	N/A	N/A	
Accelerator-Porosity Tool Wellsite Calibration - Tank Check							
Master: 24-Jul-2002 9:09							
Array-1 Standoff Porosity	11.75	11.51	N/A	N/A	N/A	N/A	PU
Array-2 Standoff Porosity	11.75	11.19	N/A	N/A	N/A	N/A	PU
Average Slowing Down Time	6.000	5.884	N/A	N/A	N/A	N/A	US
Array-1 SDT Ratio Up/Down	1.000	0.9901	N/A	N/A	N/A	N/A	
Array-2 SDT Ratio Up/Down	1.000	0.9732	N/A	N/A	N/A	N/A	
Sigma Formation	27.50	27.88	N/A	N/A	N/A	N/A	CU
Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 1 Check							
Master: 13-Jul-2002 3:08 Before: 24-Jul-2002 12:59 After: 20-Aug-2002 23:10							
Na 511 Peak Loc	40.00	40.59	40.60	40.61	0.002739	1.000	
Na 511 Peak Res	15.50	16.79	16.89	15.96	-0.9243	2.000	%
High Voltage	1150	1224	1220	1220	-0.09119	30.00	V
Na 1785 Peak Loc	142.6	145.1	146.3	145.9	-0.4483	7.000	
Na 1785 Peak Res	8.500	10.40	8.694	8.720	0.02588	2.000	%
Temperature	15.50	24.98	22.43	20.55	-1.880	N/A	DEGC
Na Count Rate	45.00	50.31	49.89	49.45	-0.4308	8.000	CPS
Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 2 Check							
Master: 13-Jul-2002 3:08 Before: 24-Jul-2002 12:59 After: 20-Aug-2002 23:10							
Na 511 Peak Loc	40.00	40.58	40.59	40.62	0.02345	1.000	
Na 511 Peak Res	15.50	16.72	16.53	16.77	0.2390	2.000	%
High Voltage	1150	1253	1250	1247	-3.122	30.00	V
Na 1785 Peak Loc	142.6	144.7	144.3	144.8	0.5048	7.000	
Na 1785 Peak Res	8.500	9.766	9.897	9.571	-0.3262	2.000	%
Temperature	15.50	24.15	21.87	20.77	-1.099	N/A	DEGC
Na Count Rate	45.00	50.19	49.39	49.43	0.03497	8.000	CPS

Hostile Natural Gamma Ray Sonde Wellsite Calibration - Ratio Of Detector 1 To Detector 2

Master: 13-Jul-2002 3:08 Before: 24-Jul-2002 12:59 After: 20-Aug-2002 23:10

Coincidence Count Rate Ratio 1.000 1.004 1.010 1.000 -0.009243 0.05000

Hostile Natural Gamma Ray Sonde Master Calibration - Detector 1 Calibration

Master: 13-Jul-2002 3:01

Na 511 Peak Set Point	40.00	41.00	--	--	--	--
Th Peak Loc	209.6	208.9	--	--	--	--
Th Peak Res	7.000	8.227	--	--	--	%
Background Count Rate	142.5	24.67	--	--	--	CPS
Gain Ratio	1.000	0.9793	--	--	--	--

Hostile Natural Gamma Ray Sonde Master Calibration - Detector 2 Calibration

Master: 13-Jul-2002 3:01

Na 511 Peak Set Point	40.00	41.00	--	--	--	--
Th Peak Loc	209.6	208.8	--	--	--	--
Th Peak Res	7.000	8.191	--	--	--	%
Background Count Rate	142.5	22.68	--	--	--	CPS
Gain Ratio	1.000	0.9792	--	--	--	--

Accelerator-Porosity Tool - Detector Plateau Settings :

Near Detector Plateau Setting 1748 V
 Far Detector Plateau Setting 2052 V
 Array Detector Plateau Setting 1969 V

Dual Induction - E / Equipment Identification

Primary Equipment:

Dual Induction Sonde	DIS - HB	442
Dual Induction Cartridge	DIC - EB	438

Auxiliary Equipment:

Mass Isolated Housing	MIH - ZA	417
-----------------------	----------	-----

Dual Induction - E Wellsite Calibration

Induction Electronics (10 kHz)

Phase	ID Elect Real Offset 10 kHz MM/M	Value	Phase	ID Elect Real Gain 10 kHz	Value	Phase	ID Elect Phase 10 kHz DEG	Value
Before		37.53	Before		0.9770	Before		10.63
	-262.8 (Minimum) 37.15 (Nominal) 337.2 (Maximum)			0.8294 (Minimum) 0.9794 (Nominal) 1.171 (Maximum)			0.6325 (Minimum) 10.63 (Nominal) 20.63 (Maximum)	
Phase	ID Elect Quad Offset 10 kHz MM/M	Value	Phase	ID Elect Quad Gain 10 kHz	Value	Phase	IM Elect Phase 10 kHz DEG	Value
Before		22.25	Before		0.9660	Before		13.27
	-277.5 (Minimum) 22.53 (Nominal) 322.5 (Maximum)			0.8193 (Minimum) 0.9693 (Nominal) 1.157 (Maximum)			3.310 (Minimum) 13.31 (Nominal) 23.31 (Maximum)	
Phase	IM Elect Real Offset 10 kHz MM/M	Value	Phase	IM Elect Real Gain 10 kHz	Value			
Before		96.05	Before		0.9527			
	-453.5 (Minimum) 96.54 (Nominal) 646.5 (Maximum)			0.8074 (Minimum) 0.9574 (Nominal) 1.140 (Maximum)				
Phase	IM Elect Quad Offset 10 kHz MM/M	Value	Phase	IM Elect Quad Gain 10 kHz	Value			
Before		94.74	Before		0.9503			
	-454.8 (Minimum) 95.18 (Nominal) 645.2 (Maximum)			0.8055 (Minimum) 0.9555 (Nominal) 1.137 (Maximum)				

Before: 24-Jul-2002 13:24

Dual Induction - E Wellsite Calibration

Induction Electronics (20 kHz)

Phase	ID Elect Real Offset 20 kHz MM/M	Value	Phase	ID Elect Real Gain 20 kHz	Value	Phase	ID Elect Phase 20 kHz DEG	Value
Before		14.85	Before		1.004	Before		9.036
	-110.3 (Minimum) 14.68 (Nominal) 139.7 (Maximum)			0.8551 (Minimum) 1.005 (Nominal) 1.207 (Maximum)			-5.718 (Minimum) 9.282 (Nominal) 24.28 (Maximum)	
Phase	ID Elect Quad Offset 20 kHz MM/M	Value	Phase	ID Elect Quad Gain 20 kHz	Value	Phase	IM Elect Phase 20 kHz DEG	Value
Before		8.842	Before		0.9923	Before		12.07
	-115.9 (Minimum) 9.089 (Nominal) 134.1 (Maximum)			0.8445 (Minimum) 0.9945 (Nominal) 1.192 (Maximum)			-2.653 (Minimum) 12.35 (Nominal) 27.35 (Maximum)	
Phase	IM Elect Real Offset 20 kHz MM/M	Value	Phase	IM Elect Real Gain 20 kHz	Value			

Before		39.82	Before		1.010	
	-184.7 (Minimum)	40.31 (Nominal)	265.3 (Maximum)	0.8587 (Minimum)	1.009 (Nominal)	1.212 (Maximum)
Phase	IM Elect Quad Offset 20 kHz	MM/M	Value	Phase	IM Elect Quad Gain 20 kHz	Value
Before		39.36	Before		1.007	
	-185.2 (Minimum)	39.80 (Nominal)	264.8 (Maximum)	0.8566 (Minimum)	1.007 (Nominal)	1.209 (Maximum)

Before: 24-Jul-2002 12:54

Dual Induction - E Wellsite Calibration											
Induction Electronics (40 kHz)											
Phase	ID Elect Real Offset 40 kHz	MM/M	Value	Phase	ID Elect Real Gain 40 kHz	Value	Phase	ID Elect Phase 40 kHz DEG	Value		
Before		9.741	Before		0.9887	Before		27.54			
	-75.43 (Minimum)	9.570 (Nominal)	94.57 (Maximum)	0.8395 (Minimum)	0.9895 (Nominal)	1.185 (Maximum)	9.068 (Minimum)	29.07 (Nominal)	49.07 (Maximum)		
Phase	ID Elect Quad Offset 40 kHz	MM/M	Value	Phase	ID Elect Quad Gain 40 kHz	Value	Phase	IM Elect Phase 40 kHz DEG	Value		
Before		5.856	Before		0.9765	Before		31.11			
	-79.10 (Minimum)	5.897 (Nominal)	90.90 (Maximum)	0.8281 (Minimum)	0.9781 (Nominal)	1.169 (Maximum)	12.68 (Minimum)	32.68 (Nominal)	52.68 (Maximum)		
Phase	IM Elect Real Offset 40 kHz	MM/M	Value	Phase	IM Elect Real Gain 40 kHz	Value					
Before		26.08	Before		1.025						
	-103.8 (Minimum)	26.19 (Nominal)	156.2 (Maximum)	0.8673 (Minimum)	1.017 (Nominal)	1.224 (Maximum)					
Phase	IM Elect Quad Offset 40 kHz	MM/M	Value	Phase	IM Elect Quad Gain 40 kHz	Value					
Before		25.86	Before		1.022						
	-104.1 (Minimum)	25.92 (Nominal)	155.9 (Maximum)	0.8649 (Minimum)	1.015 (Nominal)	1.221 (Maximum)					

Before: 24-Jul-2002 13:26

Dual Induction - E Wellsite Calibration						
SFL Electronics						
Phase	SFL Voltage Offset MV	Value	Phase	SFL Voltage Gain	Value	
Before		1.196	Before		1.016	
	-15.00 (Minimum)	0 (Nominal)	15.00 (Maximum)	0.8500 (Minimum)	1.000 (Nominal)	1.200 (Maximum)
Phase	SFL Current Offset MA	Value	Phase	SFL Current Gain	Value	
Before		0.005420	Before		0.9940	
	-0.6000 (Minimum)	0 (Nominal)	0.6000 (Maximum)	0.8500 (Minimum)	1.000 (Nominal)	1.200 (Maximum)

Before: 24-Jul-2002 12:55

Dual Induction - E Wellsite Calibration											
Electronics Calibration Changes Files/Depth Intervals:											
Phase	ID (R > 27 OHM-M)	MM/M	Value	Phase	ID (R < 27 OHM-M) %	Value	Phase	SFL (R < 1 OHM-M)	OHMM	Value	
After		0.3638	After		0.001495	After		0.0005501			
	0 (Minimum)	0 (Nominal)	0.7500 (Maximum)	0 (Minimum)	0 (Nominal)	2.000 (Maximum)	0 (Minimum)	0 (Nominal)	0.02000 (Maximum)		
Phase	IM (R > 27 OHM-M)	MM/M	Value	Phase	IM (R < 27 OHM-M) %	Value					
After		0.7499	After		0.0005737						
	0 (Minimum)	0 (Nominal)	0.7500 (Maximum)	0 (Minimum)	0 (Nominal)	2.000 (Maximum)					
Phase	SFL (R > 27 OHM-M)	MM/M	Value	Phase	SFL (R < 27 OHM-M) %	Value					
After		EXCEEDS LIMIT	1.044	After		0.0005238					
	0 (Minimum)	0 (Nominal)	0.7500 (Maximum)	0 (Minimum)	0 (Nominal)	2.000 (Maximum)					

-Drill pipe affects after calibration

After: 26-Aug-2002 0:17

Dual Induction - E Master Calibration											
Test Loop Calibration: Calibration of Internal Reference to Test Loop Standard											
Phase	Deep 10 kHz Gain Factor	Value	Phase	Deep 20 kHz Gain Factor	Value	Phase	Deep 40 kHz Gain Factor	Value			
Master		0.9956	Master		1.008	Master		1.026			
	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)		
Phase	Medium 10 kHz Gain Factor	Value	Phase	Medium 20 kHz Gain Factor	Value	Phase	Medium 40 kHz Gain Factor	Value			
		1.000			1.000			1.000			
	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)		

Master	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)	1.022	Master	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)	1.030	Master	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)	1.061
Phase	Deep 10 kHz Phase Shift			Value	Phase	Deep 20 kHz Phase Shift			Value	Phase	Deep 40 kHz Phase Shift			Value
Master				0.1143	Master				-0.1524	Master				-1.426
	-1.500 (Minimum)	0 (Nominal)	1.500 (Maximum)			-2.000 (Minimum)	0 (Nominal)	2.000 (Maximum)			-4.000 (Minimum)	-1.000 (Nominal)	2.000 (Maximum)	
Phase	Medium 10 kHz Phase Shift			Value	Phase	Medium 20 kHz Phase Shift			Value	Phase	Medium 40 kHz Phase Shift			Value
Master				-0.2558	Master				-0.9331	Master				-2.461
	-1.500 (Minimum)	0 (Nominal)	1.500 (Maximum)			-3.000 (Minimum)	-1.000 (Nominal)	1.000 (Maximum)			-5.000 (Minimum)	-2.000 (Nominal)	1.000 (Maximum)	

Master: Calibration out of date 6-Oct-2001 2:50

Dual Induction - E Master Calibration														
Sonde Error Corrections: Correction for sonde response in zero conductivity environment. (Normalized to 25C).														
Phase	Real Deep 10 kHz S.E. Corr.			Value	Phase	Real Deep 20 kHz S.E. Corr.			Value	Phase	Real Deep 40 kHz S.E. Corr.			Value
Master				44.95	Master				16.36	Master				4.690
	-50.00 (Minimum)	0 (Nominal)	125.0 (Maximum)			-30.00 (Minimum)	0 (Nominal)	30.00 (Maximum)			-15.00 (Minimum)	0 (Nominal)	15.00 (Maximum)	
Phase	Quad Deep 10 kHz S.E. Corr.			Value	Phase	Quad Deep 20 kHz S.E. Corr.			Value	Phase	Quad Deep 40 kHz S.E. Corr.			Value
Master				108.9	Master				64.63	Master				46.10
	-250.0 (Minimum)	0 (Nominal)	350.0 (Maximum)			-125.0 (Minimum)	0 (Nominal)	200.0 (Maximum)			-75.00 (Minimum)	0 (Nominal)	125.0 (Maximum)	
Phase	Real Medium 10 kHz S.E. Corr.			Value	Phase	Real Medium 20 kHz S.E. Corr.			Value	Phase	Real Medium 40 kHz S.E. Corr.			Value
Master				20.73	Master				-1.786	Master				-10.46
	-50.00 (Minimum)	0 (Nominal)	140.0 (Maximum)			-50.00 (Minimum)	0 (Nominal)	50.00 (Maximum)			-30.00 (Minimum)	0 (Nominal)	30.00 (Maximum)	
Phase	Quad Medium 10 kHz S.E. Corr.			Value	Phase	Quad Medium 20 kHz S.E. Corr.			Value	Phase	Quad Medium 40 kHz S.E. Corr.			Value
Master				-105.8	Master				-34.20	Master				11.45
	-1300 (Minimum)	0 (Nominal)	1300 (Maximum)			-650.0 (Minimum)	0 (Nominal)	650.0 (Maximum)			-350.0 (Minimum)	0 (Nominal)	350.0 (Maximum)	

Master: Calibration out of date 6-Oct-2001 3:22

Hostile Environment Litho Density - A / Equipment Identification

Primary Equipment:

HOSTILE ENVIRONMENT LITHO DENSITY HIGH V	HLDV - A	10
HOSTILE ENVIRONMENT LITHO DENSITY CARTRI	HLDC - AA	11
Gamma Source Radioactive	GSR - Z	1846

Auxiliary Equipment:

HOSTILE ENVIRONMENT LITHO DENSITY SONDE	HLDS - B	10
HOSTILE ENVIRONMENT ELECTRONICS CARTRIDG	HEH - H	12
HOSTILE ENVIRONMENT ELECTRONICS CARTRIDG	HEH - G	11
HOSTILE ENVIRONMENT LITHO DENSITY PAD	HLDP - B	10

Nuclear Porosity Lithology Cartridge - B / Equipment Identification

Primary Equipment:

NPLC Cartridge	NPLC - B	79
----------------	----------	----

Auxiliary Equipment:

NPLC Housing	NPH - B	82
--------------	---------	----

Accelerator-Porosity Tool / Equipment Identification

Primary Equipment:

Accelerator-Porosity Sonde	APS - BA	22
APS Minitron	MNTR - F	4185

Auxiliary Equipment:

Accelerator-Porosity Housing	APH - AC	22
APS Calibration Water Tank	SFT - 178	4722
APS Aluminium Calibrator Sleeve	SFT - 281	24

Hostile Natural Gamma Ray Sonde / Equipment Identification

Primary Equipment:

HNGS Sonde

HNGS - BA

77

Auxiliary Equipment:

HNGS Sonde Housing

HNSH - BA

79

Gamma Source Radioactive

GSR - U

135

Hostile Natural Gamma Ray Sonde Wellsite Calibration

Detector 1 Check

Phase	Na 511 Peak Loc	Value	Phase	Na 511 Peak Res %	Value	Phase	High Voltage V	Value
Master		40.59	Master		16.79	Master		1224
Before		40.60	Before		16.89	Before		1220
After		40.61	After		15.96	After		1220
	37.50 (Minimum) 40.00 (Nominal) 42.50 (Maximum)			12.00 (Minimum) 15.50 (Nominal) 19.00 (Maximum)			900.0 (Minimum) 1150 (Nominal) 1600 (Maximum)	
Phase	Na 1785 Peak Loc	Value	Phase	Na 1785 Peak Res %	Value	Phase	Temperature DEGC	Value
Master		145.1	Master		10.40	Master		24.98
Before		146.3	Before		8.694	Before		22.43
After		145.9	After		8.720	After		20.55
	135.0 (Minimum) 142.6 (Nominal) 150.3 (Maximum)			7.000 (Minimum) 8.500 (Nominal) 11.00 (Maximum)			-28.89 (Minimum) 15.50 (Nominal) 60.00 (Maximum)	
Phase	Na Count Rate CPS	Value						
Master		50.31						
Before		49.89						
After		49.45						
	10.00 (Minimum) 45.00 (Nominal) 100.0 (Maximum)							
Master: 13-Jul-2002 3:08			Before: 24-Jul-2002 12:59			After: 20-Aug-2002 23:10		

Hostile Natural Gamma Ray Sonde Wellsite Calibration



Detector 2 Check






Phase	Na 511 Peak Loc	Value	Phase	Na 511 Peak Res %	Value	Phase	High Voltage V	Value
Master		40.58	Master		16.72	Master		1253
Before		40.59	Before		16.53	Before		1250
After		40.62	After		16.77	After		1247
	37.50 (Minimum) 40.00 (Nominal) 42.50 (Maximum)			12.00 (Minimum) 15.50 (Nominal) 19.00 (Maximum)			900.0 (Minimum) 1150 (Nominal) 1600 (Maximum)	
Phase	Na 1785 Peak Loc	Value	Phase	Na 1785 Peak Res %	Value	Phase	Temperature DEGC	Value
Master		144.7	Master		9.766	Master		24.15
Before		144.3	Before		9.897	Before		21.87
After		144.8	After		9.571	After		20.77
	135.0 (Minimum) 142.6 (Nominal) 150.3 (Maximum)			7.000 (Minimum) 8.500 (Nominal) 11.00 (Maximum)			-28.89 (Minimum) 15.50 (Nominal) 60.00 (Maximum)	
Phase	Na Count Rate CPS	Value						
Master		50.19						
Before		49.39						
After		49.43						
	10.00 (Minimum) 45.00 (Nominal) 100.0 (Maximum)							
Master: 13-Jul-2002 3:08			Before: 24-Jul-2002 12:59			After: 20-Aug-2002 23:10		






Hostile Natural Gamma Ray Sonde Wellsite Calibration

Ratio Of Detector 1 To Detector 2

Phase	Coincidence Count Rate Ratio	Value
Master		1.004

Before		1.010
After		1.000
	0.9500 (Minimum) 1.000 (Nominal) 1.050 (Maximum)	
Master: 13-Jul-2002 3:08		
Before: 24-Jul-2002 12:59		
After: 20-Aug-2002 23:10		

Hostile Natural Gamma Ray Sonde Master Calibration									
Detector 1 Calibration									
Phase	Na 511 Peak Set Point			Value	Phase	Th Peak Loc			Value
Master				41.00	Master				208.9
	38.00 (Minimum)	40.00 (Nominal)	42.00 (Maximum)			201.0 (Minimum)	209.6 (Nominal)	218.3 (Maximum)	
					Master				8.227
						5.000 (Minimum)	7.000 (Nominal)	9.000 (Maximum)	
Phase	Background Count Rate CPS			Value	Phase	Gain Ratio			Value
Master				24.67	Master				0.9793
	20.00 (Minimum)	142.5 (Nominal)	265.0 (Maximum)			0.9400 (Minimum)	1.000 (Nominal)	1.060 (Maximum)	
Master: 13-Jul-2002 3:01									

Hostile Natural Gamma Ray Sonde Master Calibration									
Detector 2 Calibration									
Phase	Na 511 Peak Set Point			Value	Phase	Th Peak Loc			Value
Master				41.00	Master				208.8
	38.00 (Minimum)	40.00 (Nominal)	42.00 (Maximum)			201.0 (Minimum)	209.6 (Nominal)	218.3 (Maximum)	
					Master				8.191
						5.000 (Minimum)	7.000 (Nominal)	9.000 (Maximum)	
Phase	Background Count Rate CPS			Value	Phase	Gain Ratio			Value
Master				22.68	Master				0.9792
	20.00 (Minimum)	142.5 (Nominal)	265.0 (Maximum)			0.9400 (Minimum)	1.000 (Nominal)	1.060 (Maximum)	
Master: 13-Jul-2002 3:01									

Company: Lamont Doherty



Well: ODP Leg 204, Site 1250F
 Field: Hydrate Ridge
 Ocean: Pacific
 State: Oregon

Phasor Induction

Natural Gamma Ray (Tcombo)